



REVIEW ARTICLE

RECENT DEVELOPMENTS IN UV-SPECTROSCOPY TECHNIQUES FOR QUANTITATIVE ANALYSIS IN PHARMACEUTICAL DOSAGE FORMS

Ravindra Kumar Maurya^{*}, G. Pavan Kumar, Gyan Singh, Jitendra Malik, Surendra Pratap Singh, Anadi Tiwari

Faculty of Pharmacy, P.K. University, Thanra - 473665, Shivpuri, Madhya Pradesh, India.

Article History

Received: 12 November 2023

Revised: 16 December 2023

Accepted: 05 January 2024

Published: 25 March 2024

Correspondence should be addressed to

Ravindra Kumar Maurya,
Research Scholar, Faculty of
Pharmacy, PK University, Thanra -
473665, Madhya Pradesh, India.

Email- drravindra17293@gmail.com

ABSTRACT: Recent advances in UV-spectroscopy have significantly enhanced the quantitative assessment of pharmacological dosage forms by offering greater sensitivity and accuracy. This paper discusses recent developments in ultraviolet (UV) spectroscopy and how they affect drug analysis. Among the significant new advancements are nanotechnology, chemometrics, microfluidics, enhanced data processing, and smaller equipment. Scholars have used nanoparticles and nanocomposites to improve UV absorption and signal amplification. This makes selective detection possible even in complex matrices. The accuracy and resilience of data analysis and interpretation are increased by the use of chemometric techniques, such as principal component analysis and partial least squares. High-throughput analysis is possible with smaller sample volumes and less time needed thanks to miniature microfluidic technologies. Modern data processing techniques provide the possibility of spectrum analysis such as derivative spectroscopy and wavelet transform. A convenient and lightweight option for on-location analysis and point-of-care testing is the compact UV spectrophotometer. These developments have made UV spectroscopy essential for formulation development and quality control in the pharmaceutical sector. Two possible directions for the future are to better integrate these technologies for real-time analysis and to tackle novel issues in pharmaceutical analysis.

Key Words: UV-spectroscopy, Nanotechnology, Chemometrics, Microfluidics

I. INTRODUCTION

A dependable and accurate thread in the intricate web of pharmaceutical analysis is UV spectroscopy. UV spectroscopy has been there from the beginning and is one of the most significant technologies accessible to pharmaceutical researchers for researching dosage types [1]. Ultraviolet spectroscopy basically uses the unique ways that molecules absorb ultraviolet light to identify and quantify them. Among the various applications supported by this fundamental idea are the measurement of active pharmaceutical ingredients (APIs), formulation purity evaluation, and breakdown pathway clarification [2].

UV spectroscopy has various applications in pharmaceutical analysis. This approach, which does not contaminate the sample in any way, enables scientists to swiftly and securely ascertain the chemical composition of pharmaceutical formulations while also yielding critical details on the presence and amount of key components. Throughout the whole pharmaceutical lifecycle [3], from preliminary research and development to post-marketing surveillance and manufacturing quality control, this proficiency is essential. In fact, in order for regulators and stakeholders to make informed decisions about the efficacy, safety, and quality of medicinal products, UV spectroscopy is essential [4].

Given its historical relevance, recent advances at the frontier of science and technology are propelling a paradigm shift in the

use of ultraviolet (UV) spectroscopy in pharmaceutical investigation. The breadth and possibilities of UV-spectroscopy are being totally transformed by these developments, which are fueled by the pharmaceutical industry's unquenchable thirst for change [5].

By providing a thorough summary of the most recent advancements that have raised the accuracy, sensitivity, and efficiency of ultraviolet (UV) spectroscopy to new heights, this introductory part seeks to highlight the long-term significance of UV spectroscopy in pharmaceutical analysis [6]. Thanks to the integration of cutting-edge nanotechnologies, the application of sophisticated chemometric techniques, and the reduction of apparatus size, these advancements represent a significant milestone in the history of UV spectroscopy. Without an understanding of and use for these advancements, pharmaceutical researchers and practitioners would stay enmeshed in academia and unable to ensure product quality, enhance processes, and navigate the complex regulatory environment in a changing world. As we go into the unexplored realm of UV spectroscopy, we enter a world where the old and the modern clash, where tried-and-true procedures meet cutting-edge instruments, and where the unwavering pursuit of pharmaceutical analytical precision is crucial [7].

II. NANOTECHNOLOGY-ENABLED UV-SPECTROSCOPY

A. Integration of nanoparticles and nanocomposites

Through its ability to simplify the integration of nanoparticles and nanocomposites into existing techniques, nanotechnology

has created new avenues for UV spectroscopy research. When nanoparticles such as quantum dots, gold, or silver are used wisely, their special optical properties may be used to improve UV absorption and signal amplification [8]. Nanocomposites, which are composed of nanoparticles dispersed inside a

polymeric matrix, provide a similarly flexible platform for regulated UV-absorption properties. Strategies to ensure the stability and compatibility of these nanomaterials within UV-transparent matrices are being developed in order to facilitate their widespread use in pharmaceutical investigation [9].

Table 1: Comparison of nanotechnology-enabled UV-spectroscopy techniques [10-17]

<i>Technique</i>	<i>Description</i>	<i>Advantages</i>	<i>Applications</i>
Nanoparticle-enhanced UV	Utilizes nanoparticles (e.g., gold, silver) to enhance UV absorption and signal amplification.	<ul style="list-style-type: none"> ➤ Enhanced sensitivity ➤ Selective detection ➤ Signal amplification 	<ul style="list-style-type: none"> ➤ Quantitative analysis of pharmaceutical formulations ➤ Detection of trace contaminants in environmental samples ➤ Monitoring of biological analytes in complex matrices
Nanocomposite-enhanced UV	Incorporates nanoparticles dispersed in polymeric matrices to tailor UV-absorption properties.	<ul style="list-style-type: none"> ➤ Versatile UV absorption characteristics ➤ Improved compatibility and stability 	<ul style="list-style-type: none"> ➤ Quantitative analysis of multi-API formulations ➤ Monitoring of chemical processes in real time ➤ Detection of pollutants in environmental samples
Plasmonic nanostructures	Utilizes plasmonic effects in metallic nanostructures to enhance UV absorption and signal amplification.	<ul style="list-style-type: none"> ➤ High enhancement factors ➤ Tunable optical properties 	<ul style="list-style-type: none"> ➤ Surface-enhanced Raman spectroscopy (SERS) ➤ Detection of biomolecules in biological samples ➤ Label-free biosensing applications
Quantum dot-based UV	Utilizes semiconductor nanoparticles (quantum dots) to achieve tunable UV-absorption properties and high signal-to-noise ratios.	<ul style="list-style-type: none"> ➤ Narrow absorption spectra ➤ High quantum yield ➤ Photostability 	<ul style="list-style-type: none"> ➤ Bioimaging and biosensing applications ➤ Single-molecule detection ➤ Energy harvesting and optoelectronic devices
Nanoparticle-coated substrates	Utilizes nanoparticle-coated substrates to enhance UV absorption and signal amplification through surface plasmon resonance.	<ul style="list-style-type: none"> ➤ Enhanced sensitivity and specificity ➤ Multiplexing capabilities 	<ul style="list-style-type: none"> ➤ Label-free detection of biomolecules ➤ Immunoassays and DNA hybridization ➤ Environmental monitoring and food safety applications
Nanorod-enhanced UV	Utilizes elongated metallic nanoparticles (nanorods) to achieve enhanced UV absorption and signal amplification.	<ul style="list-style-type: none"> ➤ Anisotropic optical properties ➤ Strong plasmonic coupling 	<ul style="list-style-type: none"> ➤ Photothermal therapy and drug delivery ➤ Surface-enhanced spectroscopy ➤ Biosensing and bioimaging applications
Nanowire-enhanced UV	Utilizes semiconductor or metallic nanowires to enhance UV absorption and signal amplification.	<ul style="list-style-type: none"> ➤ High aspect ratio ➤ Large surface-to-volume ratio ➤ Tailorable optical properties 	<ul style="list-style-type: none"> ➤ Photodetectors and photovoltaic devices ➤ Gas and chemical sensors ➤ Bioelectronic devices
Nanofluidic UV	Integrates nanofluidic channels with UV-spectroscopic detection to manipulate and analyze nanoscale volumes of samples.	<ul style="list-style-type: none"> ➤ Precise control over sample volumes and flow rates ➤ Reduced sample consumption and waste generation 	<ul style="list-style-type: none"> ➤ Single-molecule spectroscopy and analysis ➤ DNA sequencing and genotyping ➤ Drug screening and discovery

B. Enhanced UV absorption and signal amplification

When added to UV-spectroscopy techniques, nanoparticles and nanocomposites cause a dramatic shift in UV absorption and signal amplification. Two processes by which nanomaterials exhibit enhanced UV-absorption qualities and amplify the signal are surface plasmon resonance and quantum confinement effects. This amplification enhances signal-to-noise ratios and detection limits, enabling the analysis of trace analytes with previously unheard-of detection limits. Researchers may enhance the utility of UV spectroscopy offered by nanotechnology by customising the size, shape, and surface chemistry of nanoparticles to meet specific analytical requirements [18].

C. Selective detection in complex matrices

The issues brought on by complex sample matrices may be resolved by nanotechnology-enabled UV spectroscopy by using selective detection methods. Using the distinctive optical properties of nanomaterials, such as plasmonic or photonic effects, is one method of achieving selective interactions between nanoparticles and target analytes. Because of its

selectivity, UV spectroscopy analysis may distinguish between the analytes of interest and background constituents, hence increasing its specificity. This is why UV-spectroscopy enabled by nanotechnology is used in pharmaceutical analysis, environmental monitoring, and bioanalytical studies. It allows for extremely selective detection in complex matrices [19].

D. Application examples

Numerous examples of applications in various sectors demonstrate how revolutionary UV spectroscopy enabled by nanotechnology may be. Nanotechnology in pharmaceutical analysis facilitates the quantitative analysis of multi-API formulations, resulting in improved sensitivity and specificity. Furthermore, the use of UV-spectroscopy made possible by nanotechnology, which enables the detection of trace contaminants in environmental samples, may be able to satisfy one of the most urgent needs for environmental monitoring [20]. The accomplishment of selective detection in complex biological matrices has significant ramifications for biomedical applications, providing fresh opportunities for advances in diagnosis and treatment. Online monitoring systems that use UV spectroscopy enabled by nanotechnology provide real-time

process management in industrial settings, further ensuring constant product quality. These use cases demonstrate how UV spectroscopy may be enhanced by nanotechnology for a range of analytical issues [21].

III. CHEMOMETRICS AND MULTIVARIATE ANALYSIS

A. Principles of chemometric methods:

UV-spectroscopy becomes substantially more efficient when chemometric techniques are used for data processing and

analysis. These methods extract useful information from complex datasets using a range of statistical and mathematical techniques. UV spectroscopic chemometric analysis is based on concepts such as principal component analysis (PCA), partial least squares, and cluster analysis (PLS). Chemometric techniques reduce dimensionality, identify trends, and extract crucial information from spectrum data to aid researchers in better understanding the connections between factors. As a consequence, the analytical findings are more reliable and accurate [22].

Table 2: Comparison of chemometric methods for UV-spectroscopy analysis [23-31]

<i>Chemometric Method</i>	<i>Description</i>	<i>Advantages</i>	<i>Applications</i>
Principal Component Analysis (PCA)	A statistical technique for reducing the dimensionality of spectral data while retaining most of its variance.	➤ Data reduction and visualization ➤ Identification of spectral patterns and outliers	➤ Exploratory data analysis ➤ Multivariate calibration ➤ Spectral classification
Partial Least Squares (PLS)	A regression technique that models the relationship between spectral data and analyte concentrations through latent variables.	➤ Handling of collinear and noisy data ➤ Simultaneous analysis of multiple variables	➤ Quantitative analysis of complex mixtures ➤ Calibration model development ➤ Prediction of analyte concentrations
Multivariate Curve Resolution (MCR)	A chemometric method for deconvolving complex spectral data into pure component spectra and concentration profiles.	➤ Separation of overlapping spectra ➤ Identification of individual components in mixtures	➤ Quantitative analysis of mixtures with overlapping spectra ➤ Process monitoring and control ➤ Detection of impurities and contaminants
Cluster Analysis	A technique for grouping similar spectra or samples based on their spectral features or composition.	➤ Data clustering and pattern recognition ➤ Identification of spectral classes or clusters	➤ Spectral clustering for sample classification ➤ Grouping of similar formulations or samples ➤ Spectral database organization ⁶
Discriminant Analysis	A statistical method for finding the linear combination of spectral variables that best discriminates between predefined classes or groups.	➤ Identification of spectral features that discriminate between different sample groups ➤ Prediction of sample class membership	➤ Spectral classification and pattern recognition ➤ Quality control and authentication of samples ➤ Sample classification and discrimination
Unsupervised Learning	A category of machine learning algorithms that identify patterns and relationships in spectral data without predefined class labels.	➤ Discovery of hidden structures in spectral data ➤ Data exploration and clustering	➤ Anomaly detection and outlier identification ➤ Spectral clustering and pattern recognition ➤ Exploratory data analysis
Kernel Principal Component Analysis (KPCA)	A nonlinear extension of PCA that maps spectral data into a higher-dimensional feature space for enhanced separation of classes.	➤ Nonlinear dimensionality reduction ➤ Improved separation of classes in complex datasets	➤ Spectral classification in nonlinear datasets ➤ Identification of nonlinear relationships between spectral variables
Orthogonal Partial Least Squares (OPLS)	A variant of PLS that separates predictive and orthogonal components to improve model interpretability and predictive performance.	➤ Enhanced interpretability of PLS models ➤ Improved predictive performance in noisy datasets	➤ Quantitative analysis of spectral data with complex background ➤ Calibration model optimization - ➤ Biomarker discovery
Genetic Algorithms	Optimization algorithms inspired by the process of natural selection and evolution, used for feature selection and model optimization in spectral analysis.	➤ Global optimization of spectral models ➤ Selection of relevant spectral variables	➤ Feature selection and variable reduction in spectral datasets ➤ Model optimization and calibration refinement

B. Multivariate calibration models

Multivariate calibration models, which provide a strong basis for predicting analyte concentrations in uncharacterized samples and calibrating analytical instruments, are essential to quantitative analysis in UV spectroscopy. Based on the relationship between spectral data and analyte concentrations, these models develop prediction algorithms that can accurately quantify target molecules. Common techniques include principal component analysis, multiple linear regression (MLR), and partial least squares regression (PCR). Multivariate calibration models provide for the interdependence of several

parameters, which improves the accuracy and reliability of quantitative analysis. These models take into consideration variations in sample composition and instrumental response [32].

C. Improved accuracy and robustness

When chemometric approaches are used to UV-spectroscopy, analytical results are much more reliable and accurate. By incorporating data from many spectral channels, multivariate calibration models reduce the influence of matrix effects and spectral interferences, improving the accuracy of quantitative

analysis. Chemometric techniques, which are capable of identifying even the smallest variations in the spectrum associated with analyte concentration and of identifying outliers, may further improve the accuracy of analytical findings. Thorough validation and cross-validation procedures guarantee the chemometric models' reliable performance in a variety of sample matrices and analytical environments [33].

D. Case studies

Case studies may be a powerful tool for demonstrating the efficacy and versatility of chemometric techniques in UV spectroscopy applications. This study shows that in complex sample matrices, multivariate calibration models may be used to quantify target analytes in practical scenarios. Creating calibration models for biological matrices, pharmacological formulations, or environmental samples are a few examples. Case studies highlight the benefits of integrating chemometric approaches into UV-spectroscopy procedures, which may enhance analytical performance and data quality by showcasing the practical applications of these techniques [34].

IV. MICROFLUIDIC UV-SPECTROSCOPY

A. Miniaturized platforms for high-throughput analysis

Microfluidic technologies are revolutionising UV spectroscopy by offering small, effective instruments for high-throughput research. These devices manipulate small amounts of chemicals and samples *via* microscale channels and chambers, enabling the rapid and parallel examination of several samples. Microfluidic technologies have the potential to significantly increase sample throughput and reduce the amount of time and resources required for the analysis of large sample cohorts. These technologies miniaturise analytical procedures [35].

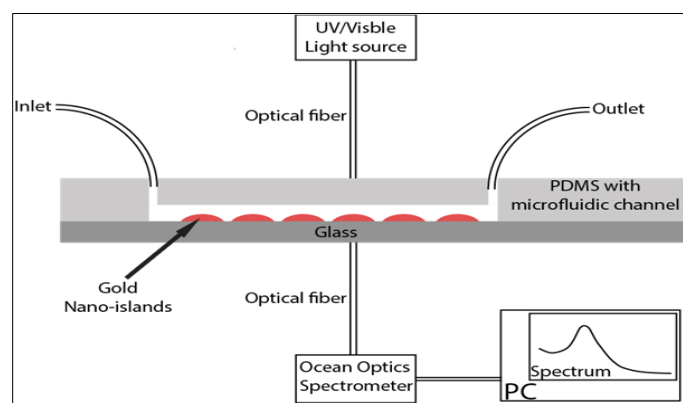


Fig. 1: Schematic representation of microfluidic UV-spectroscopy setup [36]

B. Reduced sample volumes and analysis time

One significant advantage of microfluidic UV-spectroscopy is that it may potentially operate with smaller sample amounts and shorter analysis times than traditional methods. Rapid reaction kinetics and efficient mixing are made possible by the inherent characteristics of microfluidic devices, such as laminar flow and precise fluid control, which reduce analytical times [37]. Because microfluidic UV-spectroscopy employs extremely

small sample volumes, which decrease sample consumption and waste, it is an analytical approach that is both economically and ecologically sustainable [38].

C. Integration with UV detection

Without any problems, microfluidic UV-spectroscopy seamlessly integrates UV detecting capabilities into microfluidic devices with the aim of real-time monitoring chemical and biological processes. Compact ultraviolet (UV) detectors designed for use with microfluidic systems continually gather spectrum information as samples are handled and examined. By combining the two devices, researchers can monitor reaction rates, quantify analyte concentrations, and spot changes in the spectrum instantly, enabling more accurate and flexible adjustment of the experimental conditions [39].

D. Real-time analysis applications

The monitoring capabilities of microfluidic UV-real-time spectroscopy have several applications in biotechnology, pharmaceuticals, and environmental monitoring, among other areas. Microfluidic devices in pharmaceutical research and development provide fast screening of drug formulations, investigation of reaction kinetics, and parameter control of the process. Microfluidic UV-spectroscopy is used in biotechnology for point-of-care diagnostics, biomolecular interaction studies, and enzyme kinetics research. Environmental monitoring may be used in industrial settings to monitor chemical activities, assess the quality of the water, and locate contaminants on the premises [40].

E. Illustrative examples

The examples demonstrate the wide range of applications for microfluidic UV spectroscopy. Using miniaturised UV detectors for real-time reaction monitoring in microreactors, developing instruments for high-throughput drug candidate screening, and characterising protein-ligand interactions using microfluidic UV-absorption spectroscopy are a few potential uses for microfluidic technology. These illustrations show how microfluidic UV-spectroscopy may transform analytical practises and promote creativity across a wide range of sectors [41].

V. ENHANCED DATA PROCESSING TECHNIQUES

A. Advanced algorithms for spectral analysis

New algorithms have been developed that have revolutionised spectrum analysis in UV spectroscopy by providing robust approaches for extracting relevant information from complex spectra. The employment of mathematical techniques including convolution, deconvolution, and Fourier transform by these algorithms results in improved signal-to-noise ratios, peak resolution, and detection of delicate spectrum patterns. With the use of sophisticated signal processing technologies, researchers may uncover hidden patterns, detect irregularities in the spectrum, and extract quantitative data with unmatched accuracy and precision [42].

B. Wavelet transform and derivative spectroscopy

The wavelet transform and derivative spectroscopy techniques are the most recent advancements in UV spectroscopy for enhancing spectral resolution and feature extraction. The wavelet transform separates spectral data into its frequency components so that spectral qualities may be identified at different scales. On the other hand, derivative spectroscopy highlights smaller changes in absorbance or intensity, hence highlighting greater spectral difference. By using wavelet transform and derivative spectroscopy techniques, researchers may improve the sensitivity of UV-spectroscopic analysis, make sense of overlapping peaks, and uncover hidden spectral information [43].

C. Chemometric deconvolution methods

Chemometric deconvolution algorithms are an effective method in UV spectroscopy for distinguishing overlapping peaks and interpreting complex spectra. Spectral unmixing and multivariate curve resolution are two mathematical approaches used in these methods to dissect composite spectra into their component elements (MCR). By analysing spectral data in a multivariate space, chemometric deconvolution algorithms may distinguish between signals that overlap because of several analytes or chemical species. As a consequence, researchers are able to accurately quantify the amounts of each component and ascertain their respective contributions to the spectrum [44].

D. Analysis of overlapping spectra

Overlapping spectra provide a significant challenge to UV spectroscopic research as they may lead to errors in quantification and interpretation. Modern data processing techniques, however, provide workable ways to analyse overlapping spectra and extract relevant information. Techniques like curve resolution, spectral deconvolution, and peak fitting may be used to separate overlapping signals, identify discrete components, and accurately measure their concentrations. Scientists may guarantee reliable and precise analysis of complex data by combining chemometric methods with contemporary algorithms. This enables them to take into consideration matrix effects, spectrum interferences, and other unpredictable factors [45].

Researchers now have the opportunity to possibly overcome the limitations imposed by UV-complex spectroscopy spectra thanks to new data processing technology. Spectral analysis tools, wavelet transform, derivative spectroscopy, chemometric deconvolution methods, and other sophisticated algorithms can help scientists increase spectral resolution, extract useful insights, and enhance the accuracy and dependability of UV-spectroscopic analysis in a variety of applications [46].

VI. MINIATURIZED UV-SPECTROPHOTOMETERS

A. Handheld and portable instrumentation

Miniaturized UV spectrophotometers are a major advancement in analytical instruments due to their small size, low power

consumption, and ease of use. These battery-operated, small, and light portable instruments are perfect for field measurements and analysis while on the road. With the advent of portable UV spectrophotometers, researchers may now conduct studies in remote or resource-constrained places, expanding the audience for UV spectroscopy by doing away with the need for huge, bulky laboratory apparatus and infrastructure [47].

B. Versatility in sample handling

When it comes to handling samples, miniature UV spectrophotometers are very adaptable and can readily accept a wide range of shapes and types of samples. These devices' adaptability makes it possible for researchers to analyse a variety of sample matrices without needing extensive sample preparation. They work well with materials that are semi-solid, liquid, and solid. Furthermore, on small UV spectrophotometers, cuvette holders, sample chambers, and optical attachments may be changed out to create custom setups to suit specific analytical requirements. Miniature UV spectrophotometers are becoming more and more helpful in a variety of disciplines, including pharmaceutical quality control and environmental monitoring, due to their flexibility and adaptability [48].

C. On-site analysis and point-of-care testing

Miniature UV spectrophotometers provide point-of-care testing and on-site analysis in clinical, environmental, and industrial situations, enabling rapid and decentralised testing. These portable devices may be utilised directly in the field or while samples are being gathered, eliminating the requirement for sample transfers or the usage of centralised laboratory facilities. Tiny UV spectrophotometers may be useful for environmental scientists, industrial operators, and healthcare practitioners because they can deliver real-time results that support regulatory compliance, process optimization, and decision-making. Additionally, point-of-care testing in remote or disadvantaged areas enhances healthcare outcomes and diagnostic service accessibility with the use of tiny UV spectrophotometers [49].

D. Case examples

These examples illustrate a few of the various applications and capabilities of miniature UV spectrophotometers. These devices might find use in point-of-care testing for clinical diagnostics, portable water quality monitors, and fast screening of pharmaceutical formulations for counterfeit drugs. As shown by the case studies' real-world applications, miniature UV spectrophotometers have a substantial practical value and effect in resolving analytical problems and advancing scientific research. Case examples demonstrate how miniature UV spectrophotometers are more affordable, dependable, and efficient than conventional laboratory-based instruments, and how they have the potential to completely transform analytical workflows and decision-making processes [50].

VII. CONCLUSION

Improvements in data processing, equipment shrinking, and nanotechnology have all contributed significantly to the development of UV spectroscopy techniques. Nanoparticles and nanocomposites have totally changed UV-spectroscopy by improving UV absorption, signal amplification, and selective detection in complicated matrices. Accurately quantifying analytes in overlapping spectra has been made feasible by sophisticated data processing techniques such as chemometrics, wavelet transform, and chemometric deconvolution, which have improved spectrum analysis.

Additionally, UV-spectroscopy has become more widely available because to miniature ultraviolet (UV) spectrophotometers, which enable on-site examination with previously unheard-of efficiency and mobility. These significant advancements have brought about a paradigm shift in UV spectroscopy that will enable more accessible, sensitive, and accurate pharmaceutical analysis among other applications.

These advancements will have a significant impact on pharmaceutical analysis and the future creation, testing, and assessment of medications. Pharmaceutical researchers now have new capabilities for analysing complex formulations, spotting minute contaminants, and monitoring the stability of medications in real time thanks to the use of nanotechnology in UV spectroscopy. Since analytical results are more dependable and precise, scientists may reliably draw valuable inferences from spectral data with the aid of contemporary data processing techniques. The pharmaceutical sector might undergo a significant transformation if UV spectrophotometers are made smaller, since this would allow for remote monitoring, on-site analysis, and point-of-care testing. When considered collectively, these advancements show how UV-spectroscopy has the potential to transform pharmaceutical analysis, assisting researchers in overcoming challenges related to analysis, fostering innovation, and ensuring the efficacy and security of pharmaceutical products in a field that is dynamic and complex.

Potential future directions in UV-spectroscopy for pharmaceutical analysis include investigating new nano-materials for enhanced UV absorption, signal amplification, and selective detection; developing miniaturised UV-spectrophotometers for point-of-care diagnostics and personalised medicine applications; enhancing online monitoring and process control for continuous manufacturing; and investigating novel analytical techniques like multidimensional spectroscopy for improved sensitivity and specificity.

It is hoped that these research avenues would increase pharmaceutical analysis innovation, which will expedite the creation of new medications, enhance quality control, and benefit patients.

ACKNOWLEDGEMENT: Nil

CONFLICT OF INTEREST: Nil

REFERENCES:

- Roy J. An introduction to pharmaceutical sciences: Production, chemistry, techniques and technology. Elsevier; 2011 Jul 25.
- Demchenko AP. Ultraviolet spectroscopy of proteins. Springer Science & Business Media; 2013 Nov 11.
- Brodbeck JS, Morrison LJ, Santos I. Ultraviolet photodissociation mass spectrometry for analysis of biological molecules. Chemical reviews. 2019 Dec 18;120(7):3328-80.
- Diffey BL. Sources and measurement of ultraviolet radiation. Methods. 2002 Sep 1;28(1):4-13.
- Anderson RJ, Bendell DJ, Groundwater PW. Organic spectroscopic analysis. Royal Society of Chemistry; 2004.
- Schmid FX. Biological macromolecules: UV-visible spectrophotometry. e LS. 2001 May 30.
- Raghavan R, Joseph JC. Spectroscopic Methods of Analysis: Ultraviolet and Visible Spectrophotometry. Cosmic rays. 2013;1020(10):12.
- Razzaq MY, Behl M, Nöchel U, Lendlein A. Magnetically controlled shape-memory effects of hybrid nanocomposites from oligo (ω -pentadecalactone) and covalently integrated magnetite nanoparticles. Polymer. 2014 Nov 5;55(23):5953-60.
- Ridi F, Bonini M, Baglioni P. Magneto-responsive nanocomposites: Preparation and integration of magnetic nanoparticles into films, capsules, and gels. Advances in colloid and interface science. 2014 May 1;207:3-13.
- Zeng M, Wu Y, Wang Y, Zhang Z, Fu X, Dai W. Silver nanoparticle-enhanced photocatalytic CO₂ reduction over Ag/Nb₂O₅ under UV-vis light irradiation. Applied Catalysis A: General. 2023 Sep 25;666:119412.
- Karthik K, Dhanuskodi S, Gobinath C, Prabukumar S, Sivaramakrishnan S. Multifunctional properties of microwave assisted CdO-NiO-ZnO mixed metal oxide nanocomposite: enhanced photocatalytic and antibacterial activities. Journal of Materials Science: Materials in Electronics. 2018 Apr;29:5459-71.
- Wang HU, Brandl DW, Nordlander P, Halas NJ. Plasmonic nanostructures: artificial molecules. Accounts of chemical research. 2007 Jan 16;40(1):53-62.
- Huang YM, Singh KJ, Liu AC, Lin CC, Chen Z, Wang K, Lin Y, Liu Z, Wu T, Kuo HC. Advances in quantum-dot-based displays. Nanomaterials. 2020 Jul 6;10(7):1327.
- Luo LB, Chen LM, Zhang ML, He ZB, Zhang WF, Yuan GD, Zhang WJ, Lee ST. Surface-enhanced Raman scattering from uniform gold and silver nanoparticle-coated substrates. The Journal of Physical Chemistry C. 2009 May 28;113(21):9191-6.
- Wadams RC, Yen CW, Butcher Jr DP, Koerner H, Durstock MF, Fabris L, Tabor CE. Gold nanorod enhanced organic photovoltaics: The importance of morphology effects. Organic Electronics. 2014 Jul 1;15(7):1448-57.
- Afal A, Coskun S, Emrah Unalan H. All solution processed, nanowire enhanced ultraviolet photodetectors. Applied Physics Letters. 2013 Jan 28;102(4).
- Arayanarakool R, Shui L, van den Berg A, Eijkel JC. A new method of UV-patternable hydrophobization of micro-and nanofluidic networks. Lab on a Chip. 2011;11(24):4260-6.
- Liu P, Li C, Zhang R, Tang Q, Wei J, Lu Y, Shen P. An ultrasensitive electrochemical immunosensor for procalcitonin detection based on the gold nanoparticles-enhanced tyramide signal amplification strategy. Biosensors and Bioelectronics. 2019 Feb 1;126:543-50.

19. Xia F, White RJ, Zuo X, Patterson A, Xiao Y, Kang D, Gong X, Plaxco KW, Heeger AJ. An electrochemical supersandwich assay for sensitive and selective DNA detection in complex matrices. *Journal of the American Chemical Society*. 2010 Oct 20;132(41):14346-8.
20. Malik S, Muhammad K, Waheed Y. Nanotechnology: A revolution in modern industry. *Molecules*. 2023 Jan 9;28(2):661.
21. Adams FC, Barbante C. Nanoscience, nanotechnology and spectrometry. *Spectrochimica Acta Part B: Atomic Spectroscopy*. 2013 Aug 1;86:3-13.
22. Messai H, Farman M, Sarraj-Laabidi A, Hammami-Semmar A, Semmar N. Chemometrics methods for specificity, authenticity and traceability analysis of olive oils: Principles, classifications and applications. *Foods*. 2016 Nov 17;5(4):77.
23. Maćkiewicz A, Ratajczak W. Principal components analysis (PCA). *Computers & Geosciences*. 1993 Mar 1;19(3):303-42.
24. Krishnan A, Williams LJ, McIntosh AR, Abdi H. Partial Least Squares (PLS) methods for neuroimaging: a tutorial and review. *Neuroimage*. 2011 May 15;56(2):455-75.
25. De Juan A, Jaumot J, Tauler R. Multivariate Curve Resolution (MCR). Solving the mixture analysis problem. *Analytical Methods*. 2014;6(14):4964-76.
26. Blashfield RK, Aldenderfer MS. The literature on cluster analysis. *Multivariate behavioral research*. 1978 Jul 1;13(3):271-95.
27. Brown MT, Wicker LR. Discriminant analysis. In *Handbook of applied multivariate statistics and mathematical modeling* 2000 Jan 1 (pp. 209-235). Academic Press.
28. Barlow HB. Unsupervised learning. *Neural computation*. 1989 Sep 1;1(3):295-311.
29. Nguyen M, Torre F. Robust kernel principal component analysis. *Advances in Neural Information Processing Systems*. 2008;21.
30. Boccard J, Rutledge DN. A consensus orthogonal partial least squares discriminant analysis (OPLS-DA) strategy for multiblock Omics data fusion. *Analytica chimica acta*. 2013 Mar 26;769:30-9.
31. Holland JH. Genetic algorithms. *Scientific american*. 1992 Jul 1;267(1):66-73.
32. Beebe KR, Kowalski BR. An introduction to multivariate calibration and analysis. *Analytical Chemistry*. 1987 Sep 1;59(17):1007A-17A.
33. Yang YY, Rashtchian C, Zhang H, Salakhutdinov RR, Chaudhuri K. A closer look at accuracy vs. robustness. *Advances in neural information processing systems*. 2020;33:8588-601.
34. Kharbach M, Alaoui Mansouri M, Taabouz M, Yu H. Current application of advancing spectroscopy techniques in food analysis: data handling with chemometric approaches. *Foods*. 2023 Jul 19;12(14):2753.
35. Pereira SA, Dyson PJ, Saraiva ML. Miniaturized technologies for high-throughput drug screening enzymatic assays and diagnostics—A review. *TrAC Trends in Analytical Chemistry*. 2020 May 1;126:115862.
36. Bathini S, Raju D, Badilescu S, Packirisamy M. Microfluidic plasmonic bio-sensing of exosomes by using a gold nano-island platform. *International Journal of Biomedical and Biological Engineering*. 2018 Apr 3;12(5):236-9.
37. Kent NJ, Basabe-Desmonts L, Meade G, MacCraith BD, Corcoran BG, Kenny D, Ricco AJ. Microfluidic device to study arterial shear-mediated platelet-surface interactions in whole blood: reduced sample volumes and well-characterised protein surfaces. *Biomedical microdevices*. 2010 Dec;12:987-1000.
38. Górecki T. Effect of sample volume on quantitative analysis by solid-phase microextraction Part 1. Theoretical considerations. *Analyst*. 1997;122(10):1079-86.
39. Rebordão G, Palma SI, Roque AC. Microfluidics in gas sensing and artificial olfaction. *Sensors*. 2020;20(20):5742.
40. Chen Q, An Y, Feng M, Li J, Li Y, Tong F, Qu G, Sun Z, Wang Y, Luo G. An enzyme-assembled gel monolithic microreactor for continuous flow asymmetric synthesis of aryl alcohols. *Green Chemistry*. 2022;24(24):9508-18.
41. Nge PN, Rogers CI, Woolley AT. Advances in microfluidic materials, functions, integration, and applications. *Chemical reviews*. 2013 Apr 10;113(4):2550-83.
42. Ghil M, Taricco C. Advanced spectral-analysis methods. In *Past and present variability of the solar-terrestrial system: measurement, data analysis and theoretical models 1997* (pp. 137-159). Ios Press.
43. Zheng J, Tang Z, He Y, Guo L. Sensitive detection of weak absorption signals in photoacoustic spectroscopy by using derivative spectroscopy and wavelet transform. *Journal of Applied Physics*. 2008 May 1;103(9).
44. Zekavat B, Solouki T. Chemometric data analysis for deconvolution of overlapped ion mobility profiles. *Journal of the American Society for Mass Spectrometry*. 2012 Sep 5;23(11):1873-84.
45. Brown JQ, Vishwanath K, Palmer GM, Ramanujam N. Advances in quantitative UV-visible spectroscopy for clinical and pre-clinical application in cancer. *Current opinion in biotechnology*. 2009 Feb 1;20(1):119-31.
46. Zhou P, Zhao Z, Huo HY, Liu Z. Retrieval of photometric parameters of minerals using a self-made multi-angle spectrometer based on the Hapke radiative transfer model. *Remote Sensing*. 2021 Aug 1;13(15):3022.
47. Capitan-Vallvey LF, Palma AJ. Recent developments in handheld and portable optosensing—A review. *Analytica chimica acta*. 2011 Jun 24;696(1-2):27-46.
48. Allicock OM, Yolda-Carr D, Earnest R, Breban MI, Vega N, Ott IM, Kalinich C, Alpert T, Wyllie AL. Method versatility in RNA extraction-free PCR detection of SARS-CoV-2 in saliva samples. *Progress in Biophysics and Molecular Biology*. 2023 Jun 25.
49. Chan HN, Tan MJ, Wu H. Point-of-care testing: applications of 3D printing. *Lab on a Chip*. 2017;17(16):2713-39.
50. Bacon CP, Mattley Y, DeFrece R. Miniature spectroscopic instrumentation: Applications to biology and chemistry. *Review of Scientific Instruments*. 2004 Jan 1;75(1):1-6.

How to Cite this article:

Maurya RK, Kumar GP, Singh G, Malik J, Singh SP, Tiwari A. Recent developments in UV-spectroscopy techniques for quantitative analysis in pharmaceutical dosage forms. *International Journal of Pharmaceutical Science and Medicine* 2024; 2(1): 21-27. DOI: 10.70199/IJPSM.2.1.21-27